


Calibration Certificate

Description :	Weight	Class :	F1
Capacity :	1mg-100g	Quantity :	21pc
Tracing :	1911201	Density :	7.90kg/dm ³
Release Date :	Sep-2019	Material :	Stainless Steel

Calibration Regulation: OIML R111-1:2004(E)

Notice of using weights

- 1、If you have any doubt about the weights, please send them to professional institute for further test.
- 2、Please be very careful when picking up and putting down the weights.
- 3、Hand-touching is strictly forbidden, the right using method : please with tweezer or fork and hands wear gloves.
- 4、Before using, dust on weights surface should be cleaned with professional brush or wipe.
- 5、Jingle or falling down is strictly forbidden, to avoided any scratch.
- 6、No touch any sharp object.
- 7、The weight of set can't be mixed with other weight.
- 8、The weights should be kept properly and carefully. Any dusty or wet place not suitable for stocking.

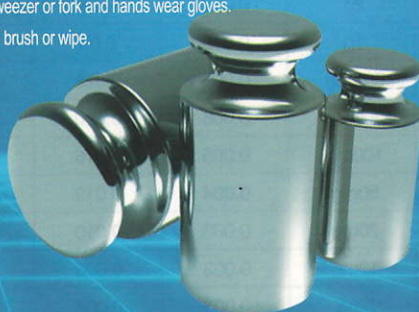

CHANGZHOU ACCURATE WEIGHT CO.,LTD

Address: NO.96 East Xingcheng Road, Bieqiao Town, Liyang City, Jiangsu, China

TEL: 86-519-87876188

Fax: 86-519-87876388

Email: sales@accurate.cc

Http://www.accurate.cc

OIML R111-1:2004(E) Tolerance Table $\pm$ mg

Denomination	OIML R111 Tolerance Table $\pm$ mg					
	E1	E2	F1	F2	M1	M2
5000kg			25000	80000	250000	800000
2000kg			10000	30000	100000	300000
1000kg		1600	5000	16000	50000	160000
500kg		800	2500	8000	25000	80000
200kg		300	1000	3000	10000	30000
100kg		160	500	1600	5000	16000
50kg	25	80	250	800	2500	8000
20kg	10	30	100	300	1000	3000
10kg	5	16	50	160	500	1600
5kg	2.5	8.0	25	80	250	800
2kg	1	3.0	10	30	100	300
1kg	0.5	1.6	5.0	16	50	160
500g	0.25	0.8	2.5	8.0	25	80
200g	0.1	0.3	1.0	3.0	10	30
100g	0.05	0.16	0.5	1.6	5.0	16
50g	0.03	0.10	0.3	1.0	3.0	10
20g	0.025	0.08	0.25	0.8	2.5	8.0
10g	0.020	0.06	0.20	0.6	2.0	6.0
5g	0.016	0.05	0.16	0.5	1.6	5.0
2g	0.012	0.04	0.12	0.4	1.2	4.0
1g	0.010	0.03	0.10	0.3	1.0	3.0
500mg	0.008	0.025	0.08	0.25	0.8	2.5
200mg	0.006	0.020	0.06	0.20	0.6	2.0
100mg	0.005	0.016	0.05	0.16	0.5	1.6
50mg	0.004	0.012	0.04	0.12	0.4	
20mg	0.003	0.010	0.03	0.10	0.3	
10mg	0.003	0.008	0.025	0.08	0.25	
5mg	0.003	0.006	0.020	0.06	0.20	
2mg	0.003	0.006	0.020	0.06	0.20	
1mg	0.003	0.006	0.020	0.06	0.20	

CHANGZHOU ACCURATE WEIGHT CO., LTD

Address: NO.88 East Xingcheng Road, Biediao Town, Lijiang City, Jiangsu, China

TEL: 86-519-87878188 FAX: 86-519-87878388
Email: sales@accurate.cc Http://www.accurate.cc